



## **Closed-Loop and Semi Closed-Loop Strategies for Control of Blood Glucose in People with Type 1 Diabetes**

**Boiroux, Dimitri; Finan, Daniel Aaron; Jørgensen, John Bagterp; Poulsen, Niels Kjølstad; Madsen, Henrik**

*Publication date:*  
2011

*Document Version*  
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

*Citation (APA):*  
Boiroux, D., Finan, D. A., Jørgensen, J. B., Poulsen, N. K., & Madsen, H. (2011). *Closed-Loop and Semi Closed-Loop Strategies for Control of Blood Glucose in People with Type 1 Diabetes*. Poster session presented at Advanced Technologies and Treatment for Diabetes 2011.

---

### **General rights**

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

## Abstract

### Comparison between 4 insulin administration strategies


- Nonlinear model predictive control (NMPC) without meal announcement.
- NMPC with meal announcement in advance.
- NMPC with meal announcement at mealtime.
- Feedforward-feedback controller.

## Feedforward-feedback controller

- A time-varying reference signal based on meal announcement reduces the risk of hypoglycemia
- Feedback from a glucose sensor
- Differentiate between basal insulin and boluses
  - Basal insulin compensates for small mismatches
  - Boluses are given at mealtimes

## Nonlinear Model Predictive Control (NMPC)

Principle of model predictive control and receding horizon

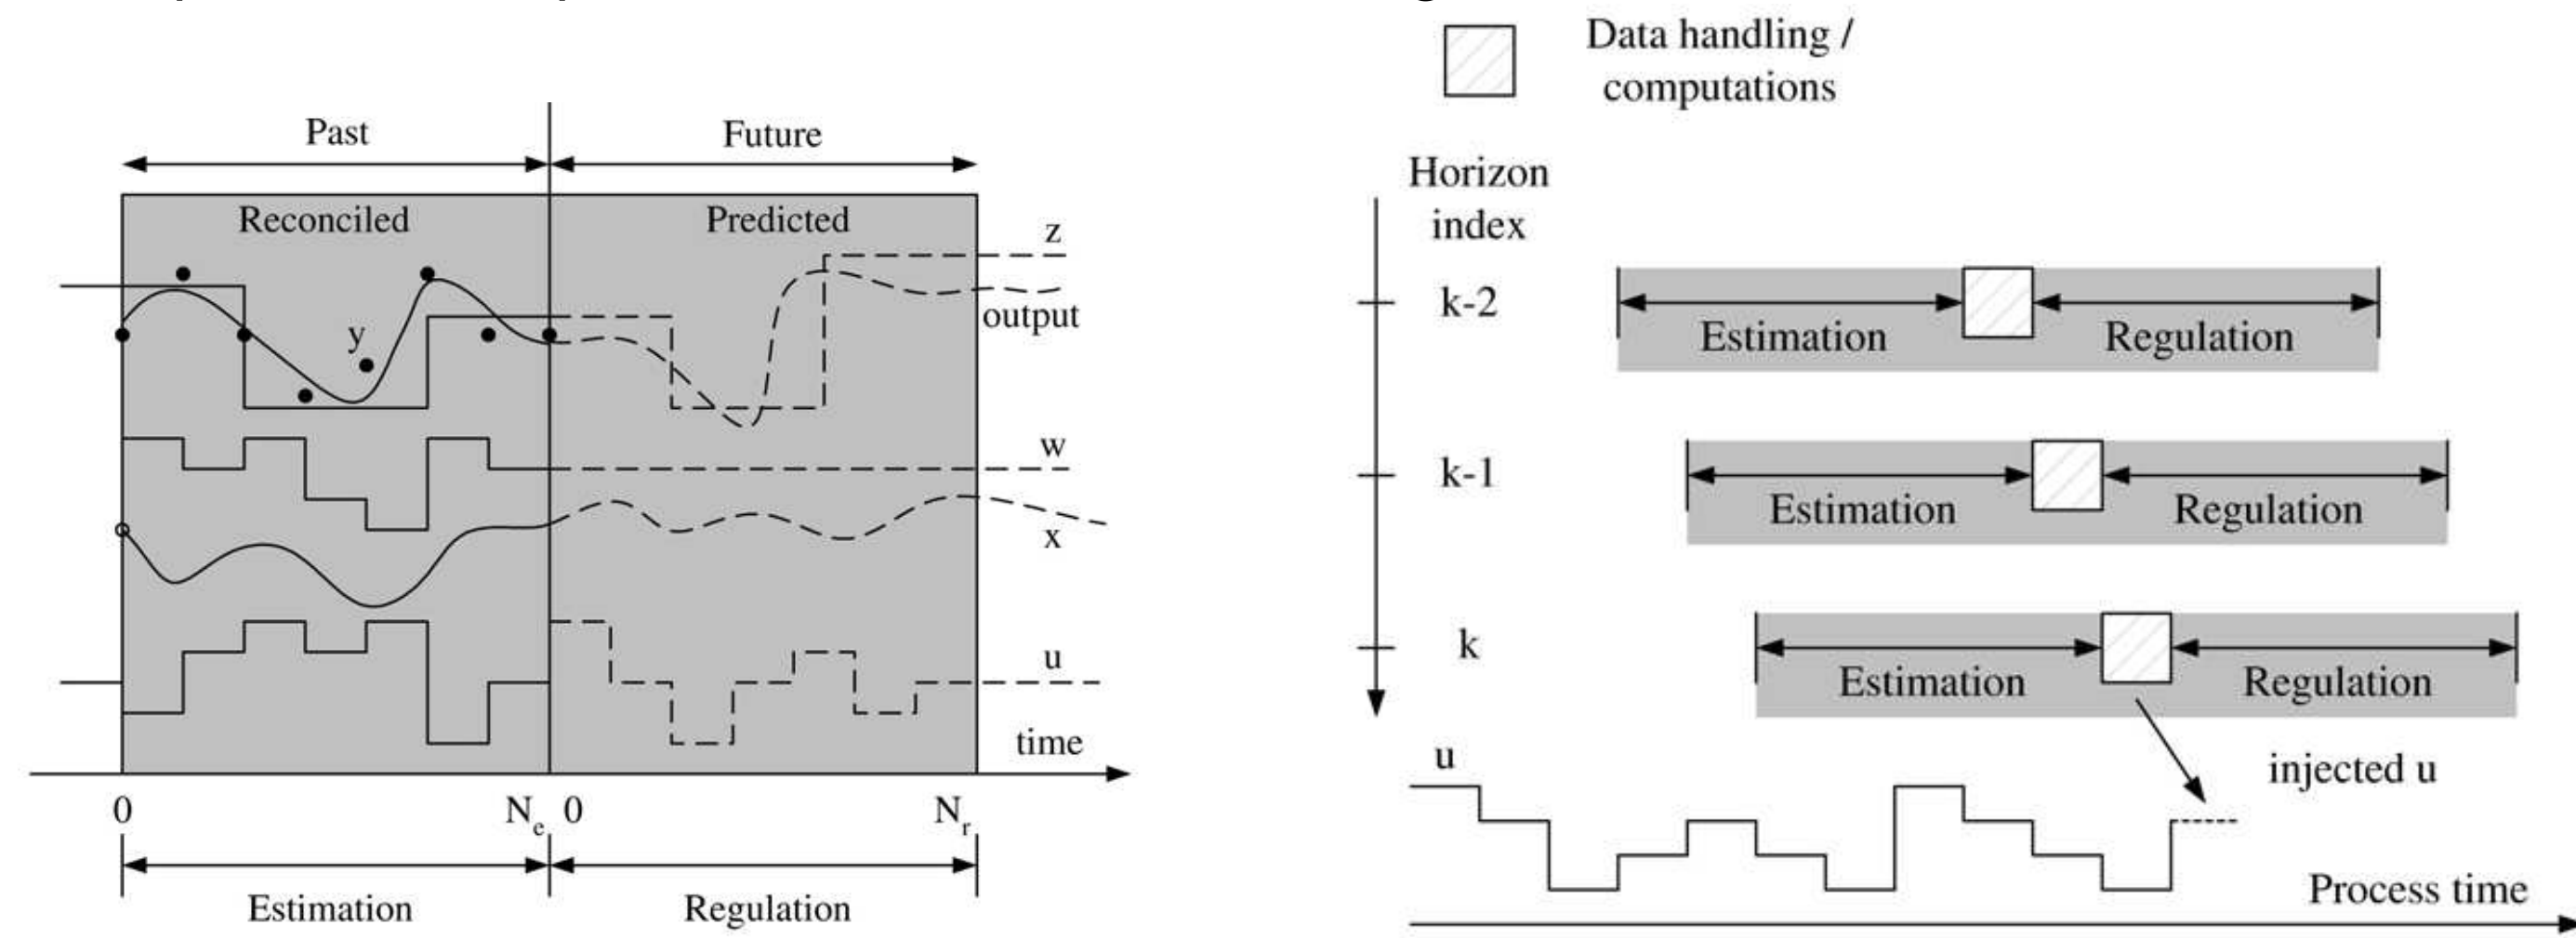

Discrete-time formulation

$$\min_{\{u_k\}_{k=0}^{N-1}} \phi = \frac{1}{2} \sum_{k=0}^{N-1} \int_{t_k}^{t_{k+1}} g(x(t), u(t)) dt$$

$$s.t. \quad \begin{aligned} x(t_0) &= x_0 \\ \dot{x}(t) &= f(x(t), u(t), d(t)) \\ y(t) &= g(x(t)) \\ u(t) &= u_k \quad t_k \leq t < t_{k+1} \end{aligned}$$

$$\begin{aligned} u_{\min} &\leq u_k \leq u_{\max} \\ \Delta u_{\min} &\leq \Delta u_k \leq \Delta u_{\max} \end{aligned}$$

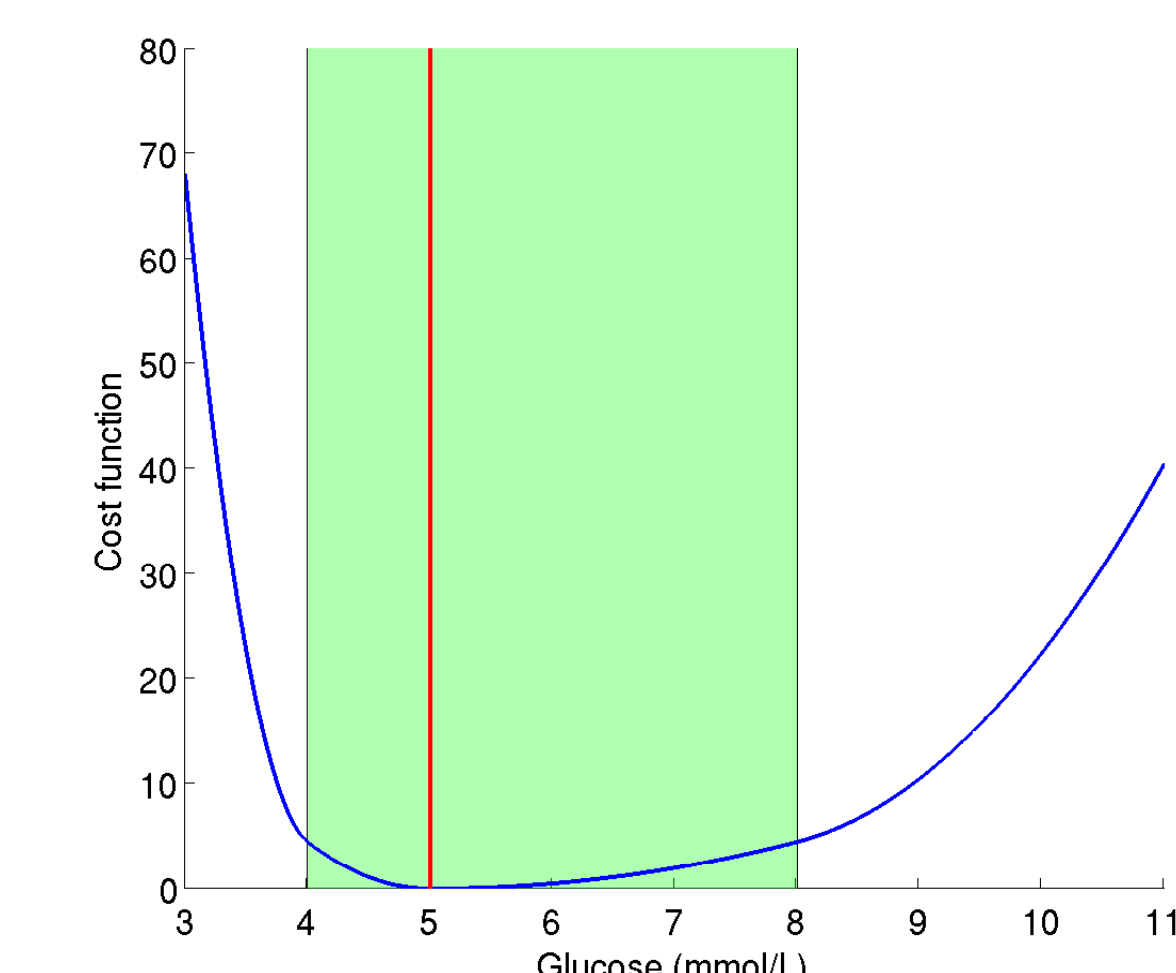


Figure 1: The cost function.

## Numerical simulations of NMPC

### Scenario

#### Meal sizes and times

- Breakfast 62g CHO at 6AM
- Lunch 55g CHO at 12PM
- Dinner 50g CHO at 6PM

### Simulations

#### Insulin administration strategies

- Meals are not announced.
- Meals are announced in advance.
- Meals are announced at mealtimes only.

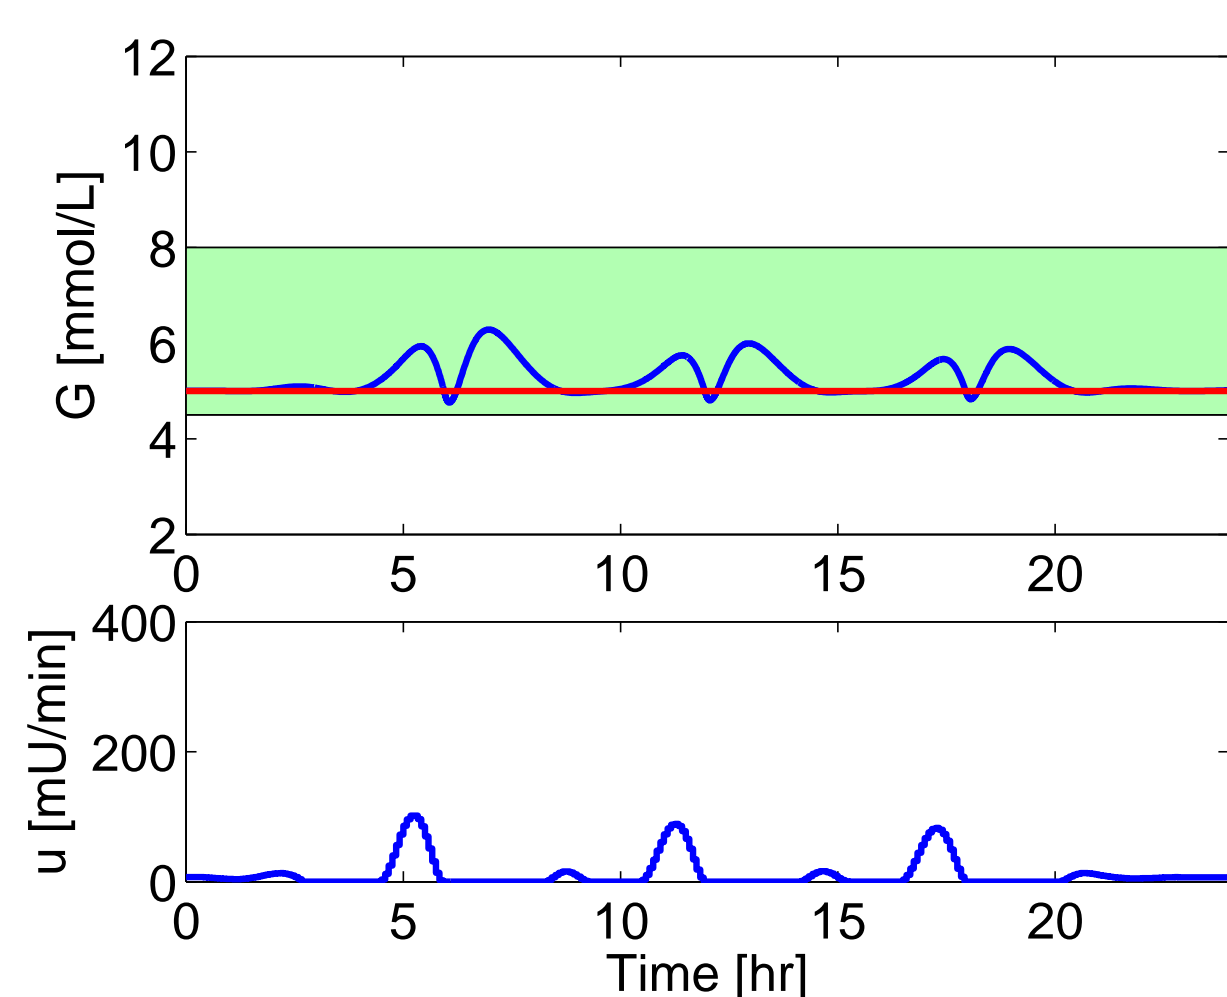


Figure 3: The case with meal announcement in advance of the meal.

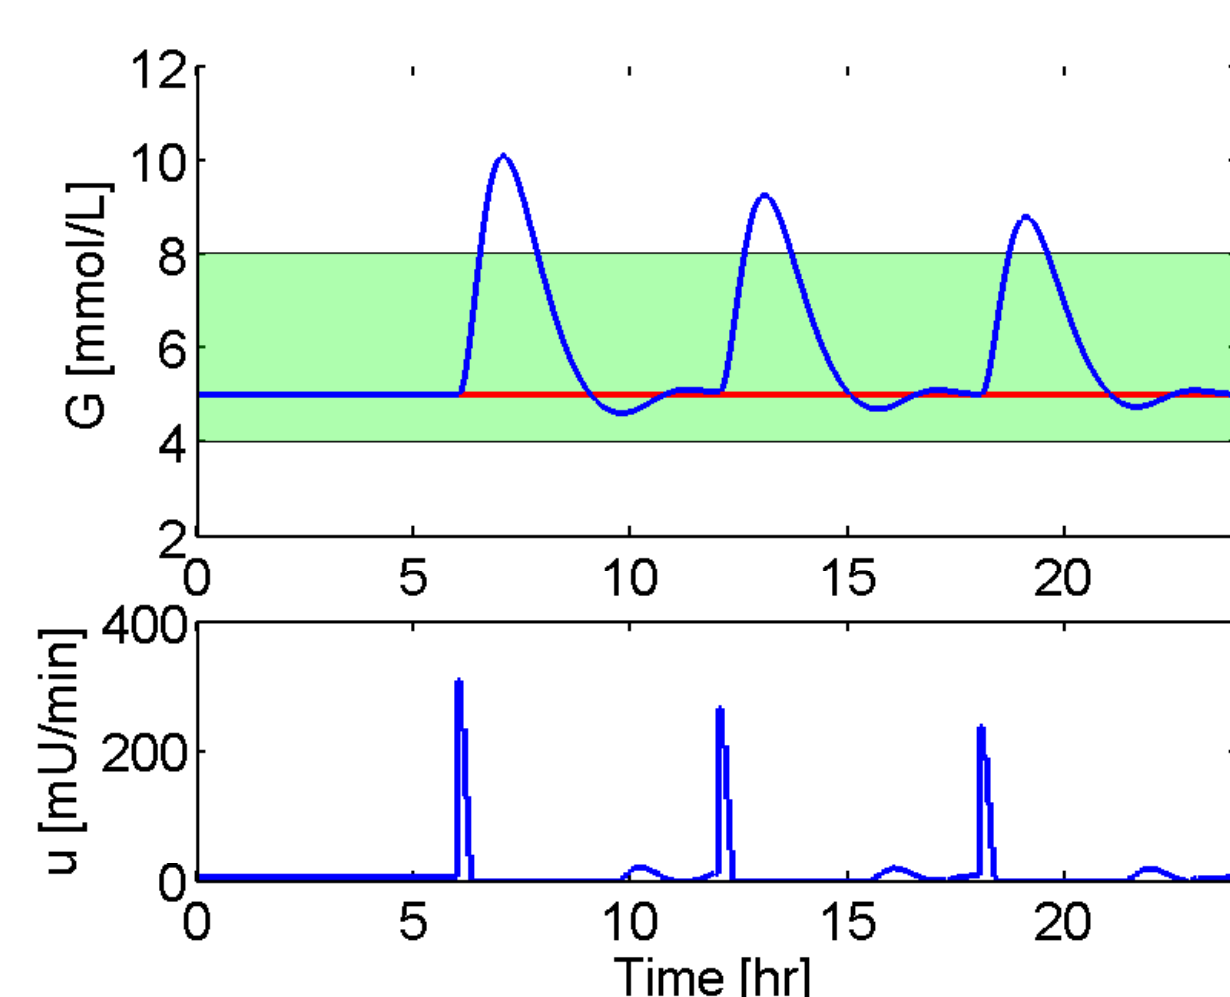


Figure 4: The case with meal announcement at mealtimes.

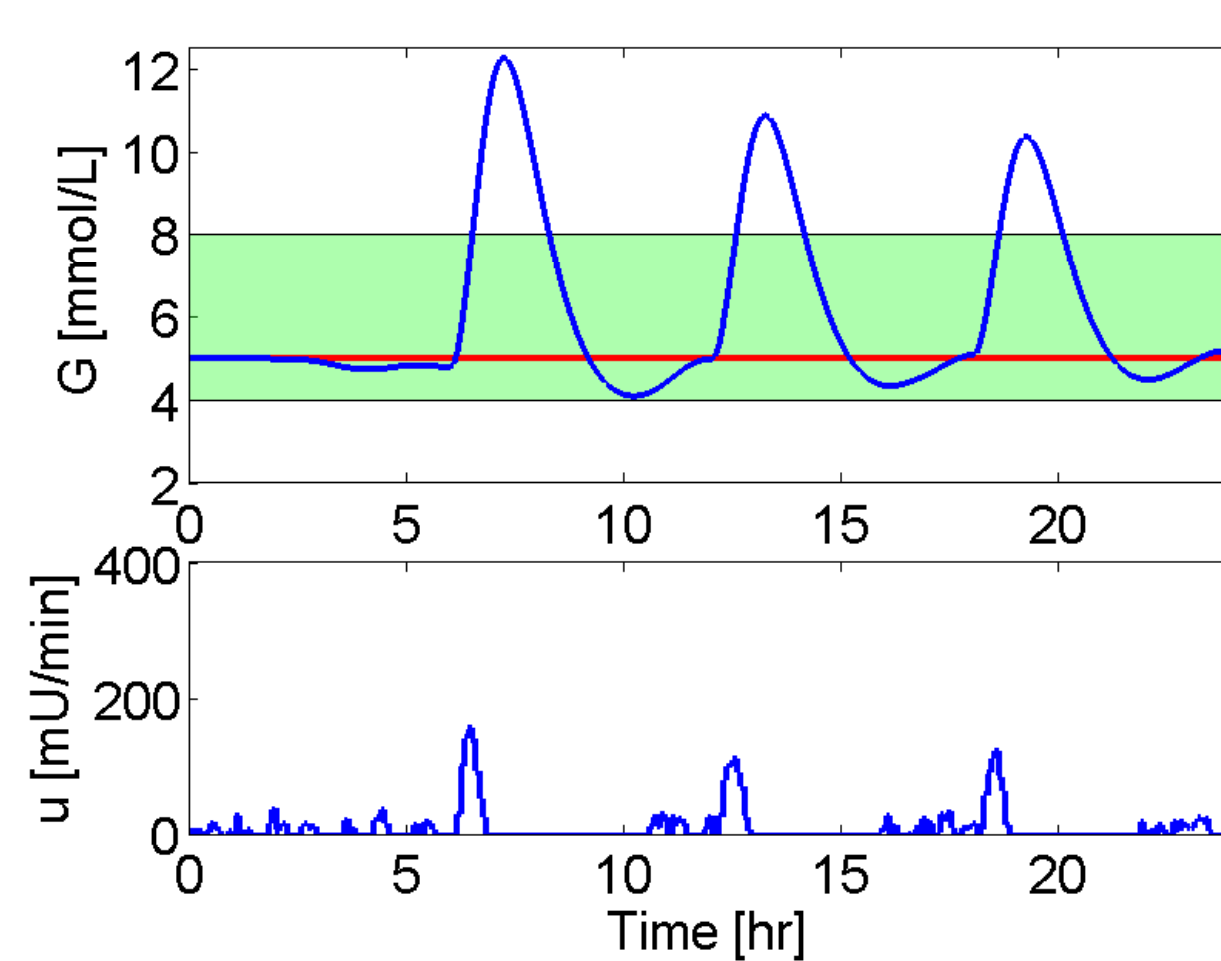


Figure 2: The case without meal announcement.

## Numerical simulations of the feedforward-feedback controller

### Scenarios

- A decrease by 50% in insulin sensitivity while fasting
- A 75g CHO meal with sensor noise
  - right meal announcement
  - meal size underestimated by 50%
  - meal size overestimated by 50%

### Simulations

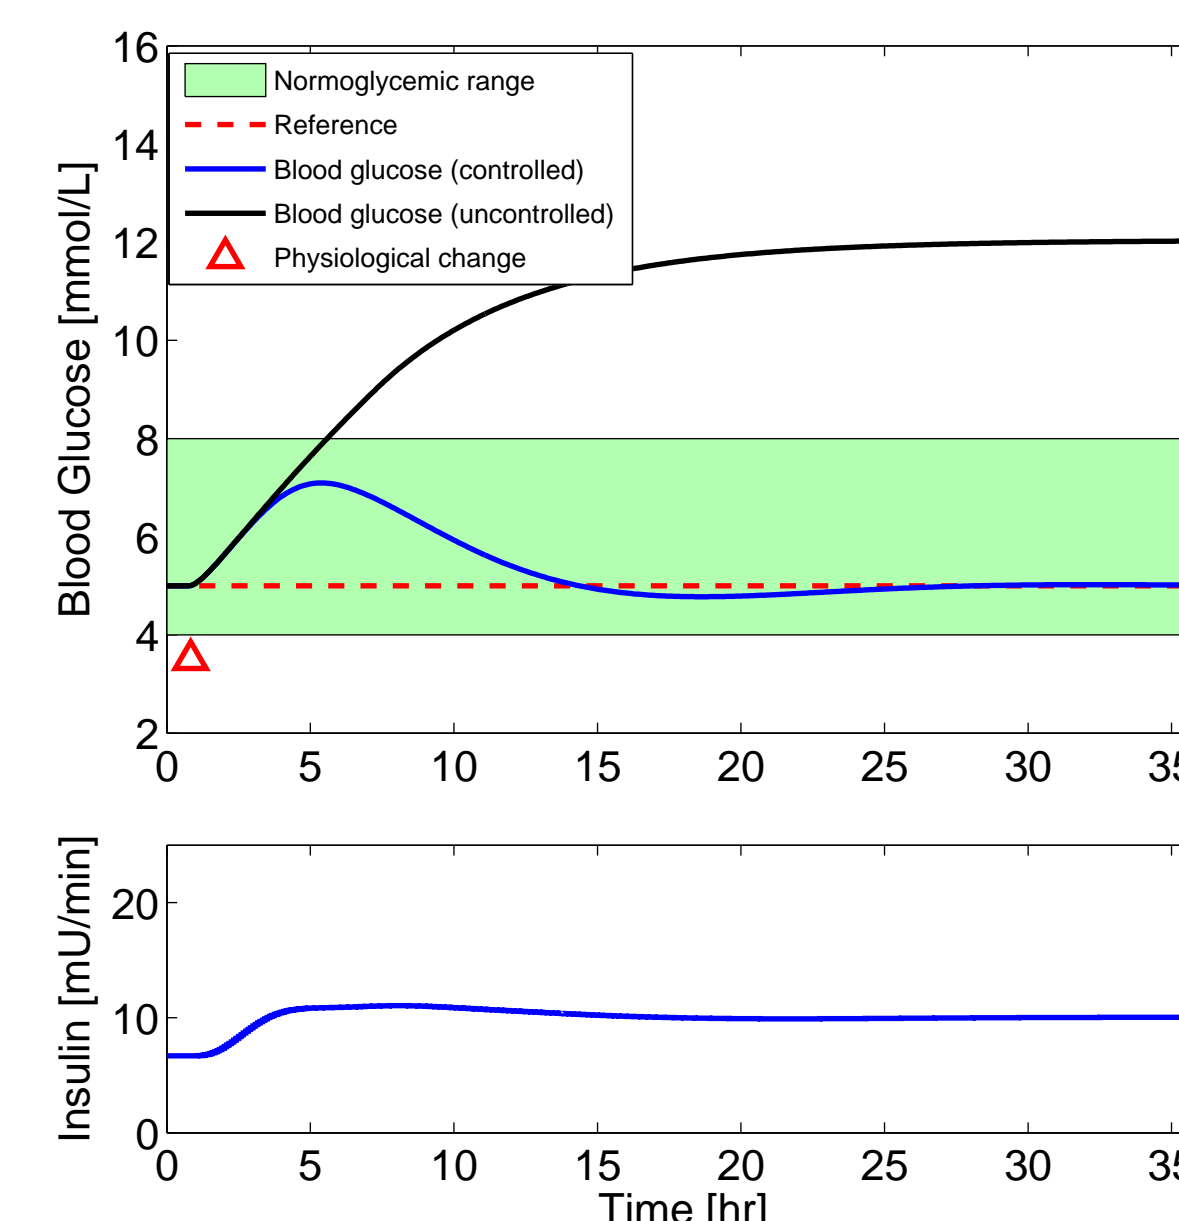


Figure 5: Insulin sensitivity is decreased by 50%.

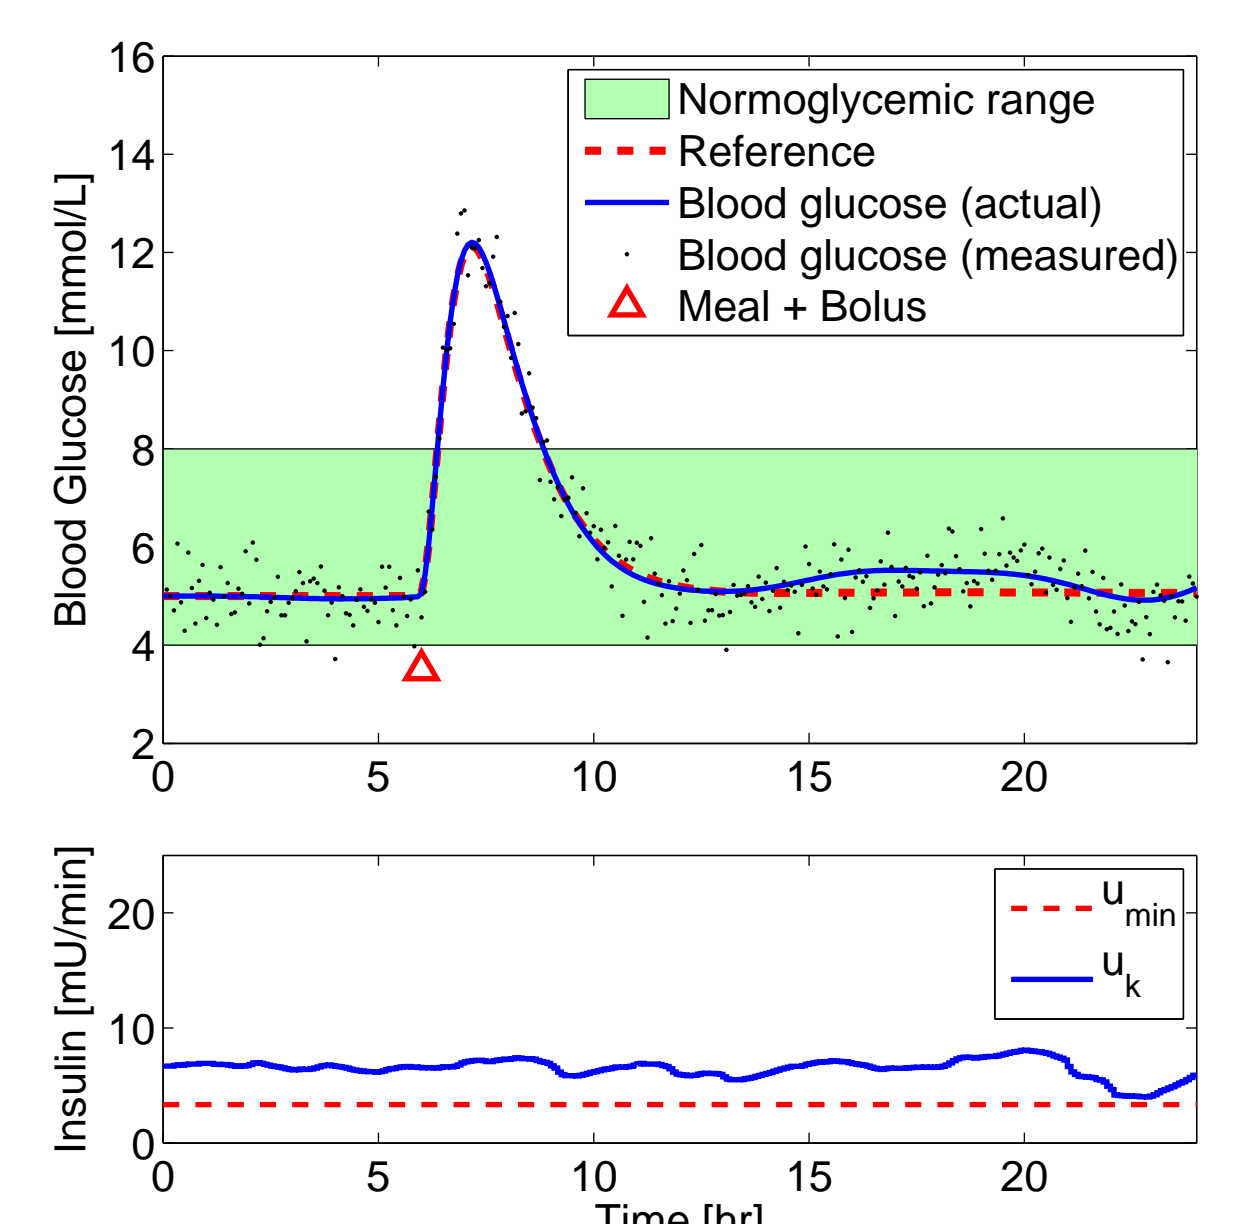


Figure 6: Exact meal size announced.

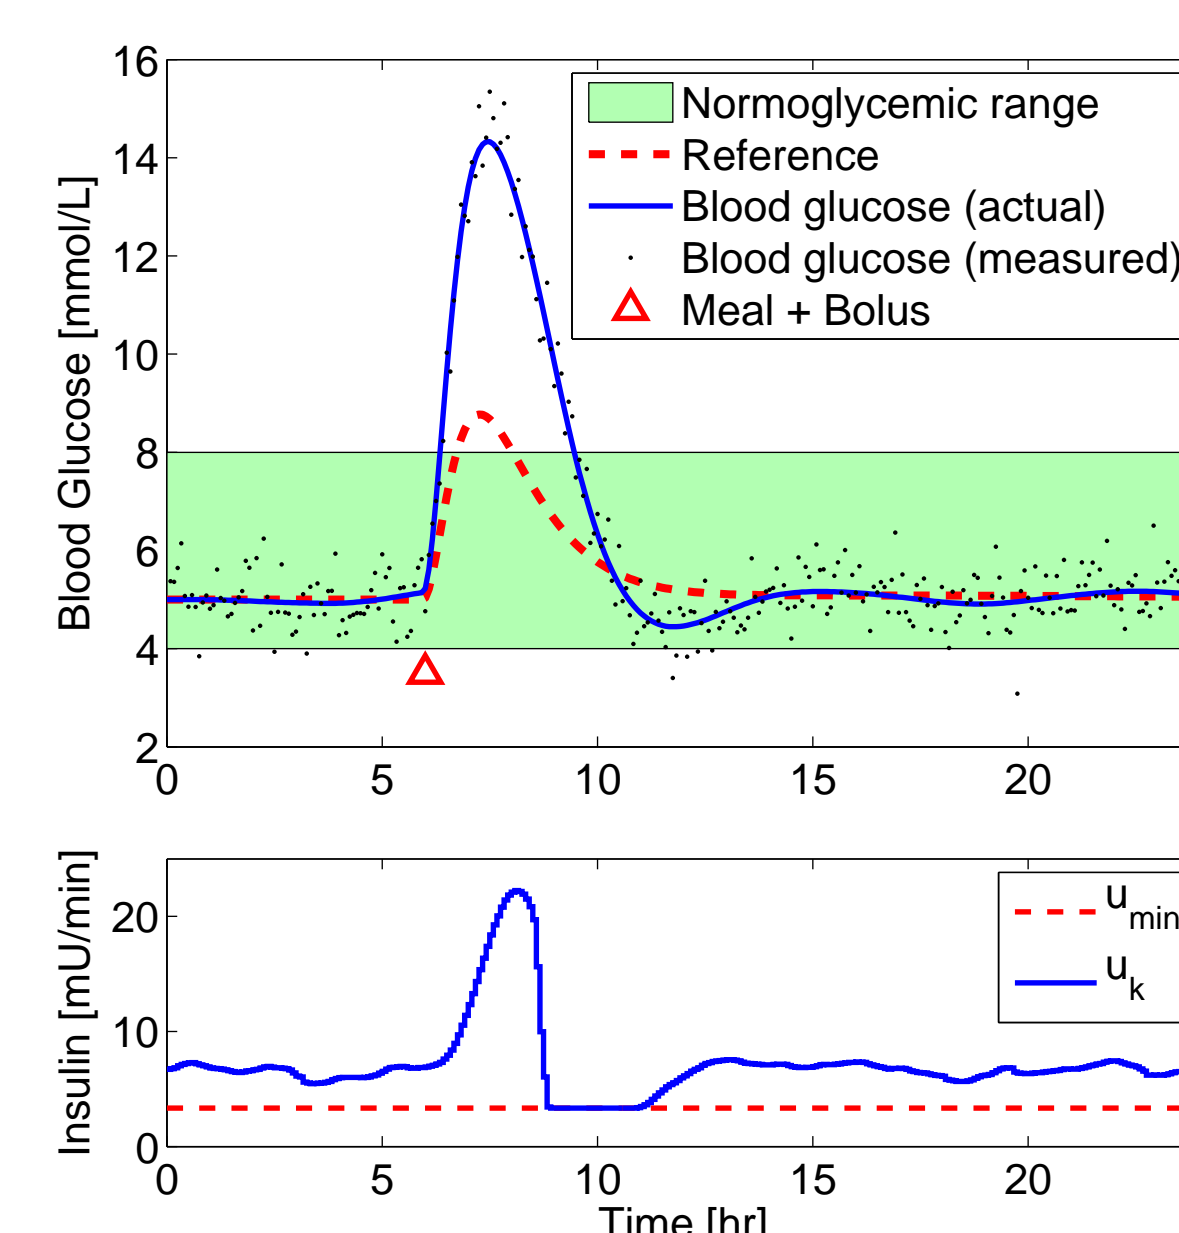


Figure 7: Meal size underestimated by 50%.

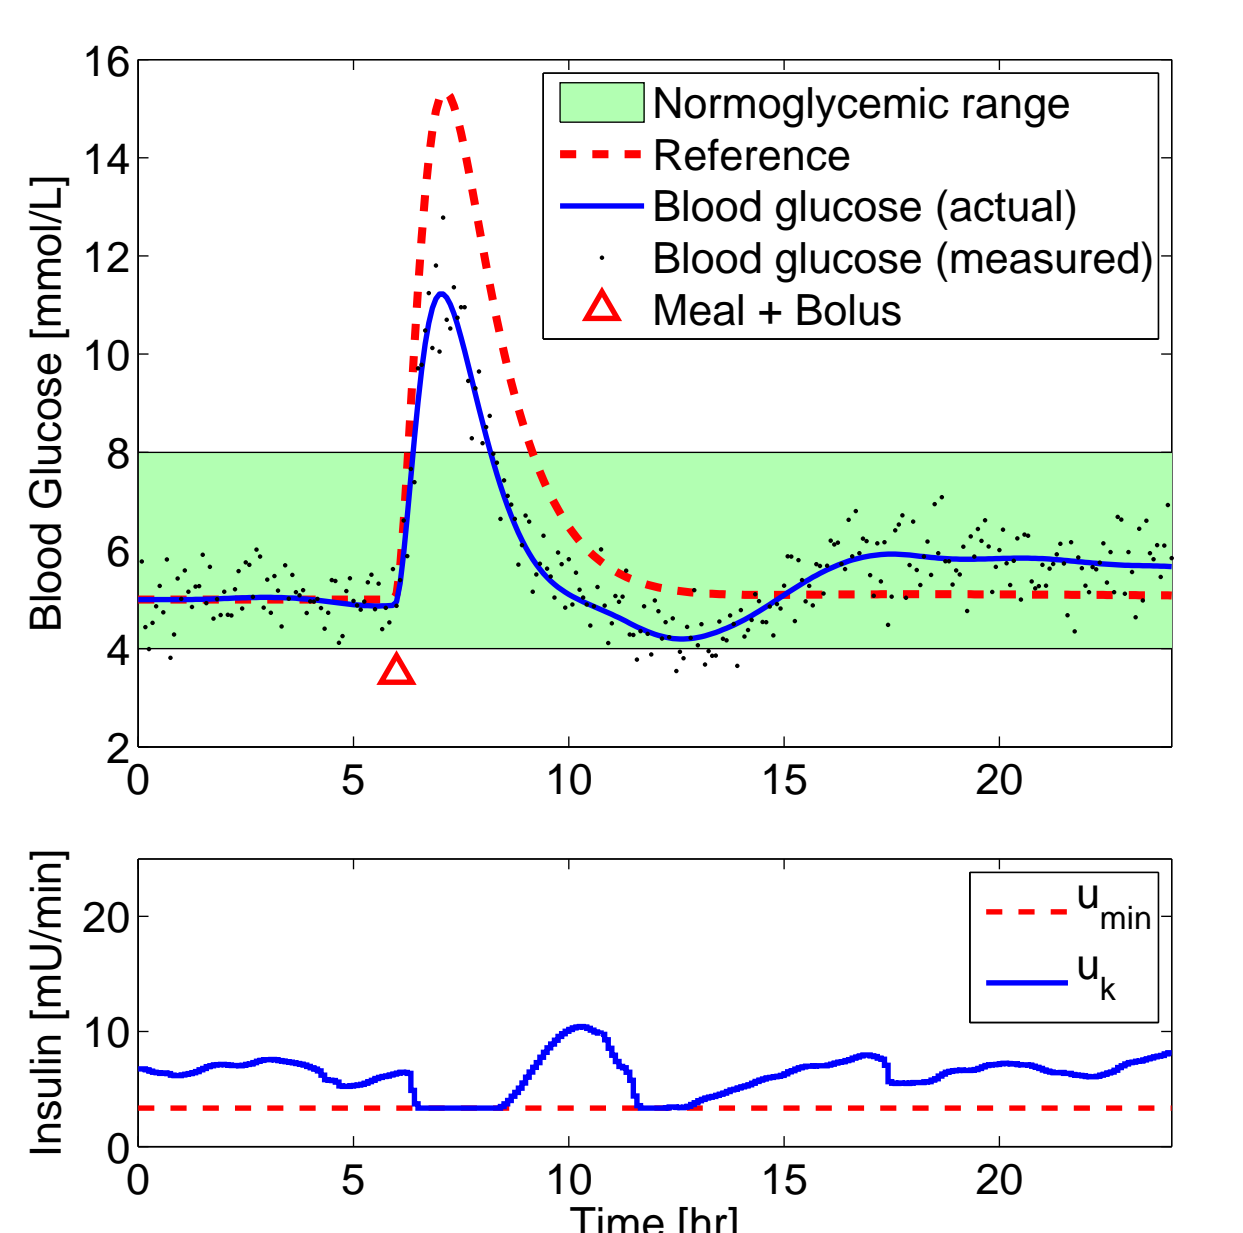


Figure 8: Meal size overestimated by 50%.

## Conclusion

- NMPC simulations give an upper-bound on the maximal achievable performance for different meal announcement strategies.
- Utilization of the bolus-like nature of the optimal insulin profile to design a feedforward-feedback controller based on linear MPC.
- Demonstration of the robustness of the feedforward-feedback controller wrt. changes in insulin sensitivity and mismatches in meal announcement in the case where an accurate enough model of the patient is available.